

All Bidders

Amendment -II

Subject: Supply, Installation, Testing & Commissioning of Bio Medical Waste Management System for PGI Satellite Centre, Sangrur, Punjab.

IFB No. : HSCC/SES/BMWMS/PGI/SANGRUR/2018 dated 09.11.2018

This has reference to above IFB.


The following Amendment may be noted which shall be treated as part of the tender document and to be submitted duly signed & stamp along with tender.

Sr. No.	Bidder's Queries	Reply
1	<p>Page No. 1 Volume IV :</p> <p>Scope of Work: Supply, Installation, Testing & Commissioning of Bio Medical Waste Management System and Turnkey work and handing over to Client.</p> <p>We request you to kindly consider Integrated Sterilizer and Shredder (ISS). This system is with new technology and having many latest features which are more productive. It has also been approved by Central Pollution Control Board as it is already in market for last 5 years and tried and tested. Operation is low and also less space is required.</p>	<p>Tender terms and conditions remain unchanged.</p>
2	<p>Page No. 6 of Volume IV:</p> <p>Contractor must take consideration in its bid, cost to be incurred for any additional work pertaining to Civil, Electrical, Plumbing, Sanitary and any other protections relevant as per State/ Central Govt. regulations/ local authority of office furniture, Service stabilizers, UPS, etc. required for successful installation testing & commissioning of the system and offered price should include all such costs, each Schedule to be considered a package in itself and contractor to execute the order package on a "turnkey basis".</p> <p>We request you to kindly provide drawing/layout.</p>	<p>Tender terms and conditions remain unchanged.</p> <p>Layout drawings attached.</p>

3	<p>PGIMER Chandigarh has already tendered for integrated sterilizer and shredder for treatment of biomedical waste. It is only advisable that its satellite centre also goes for the latest technology and not antiquated and outdated technology like separate autoclave and separate shredder which not only occupies more space and time to complete a cycle but also is lower in efficiency of sterilization & shredding and requires more manpower.</p> <p>We suggest 1 x 150 ltrs integrated sterilizer is enough for this hospital instead of the 400ltr autoclave and shredder asked in the tender as the cycle time of the integrated system is 1/3rd as that of separate system. Space requirement for the same would only be 7 ft x 7ft x 7ft. For specifications of the system PGIMER tender maybe referred to or we may provide tender specifications of other government hospitals who has installed the integrated system.</p>	Tender terms and conditions remain unchanged.
---	---	---

All other terms & conditions remain unchanged.

Sr. Chief General Manager -I, HSCC (I) Ltd.
For and behalf of Director, PGIMER, Chandigarh

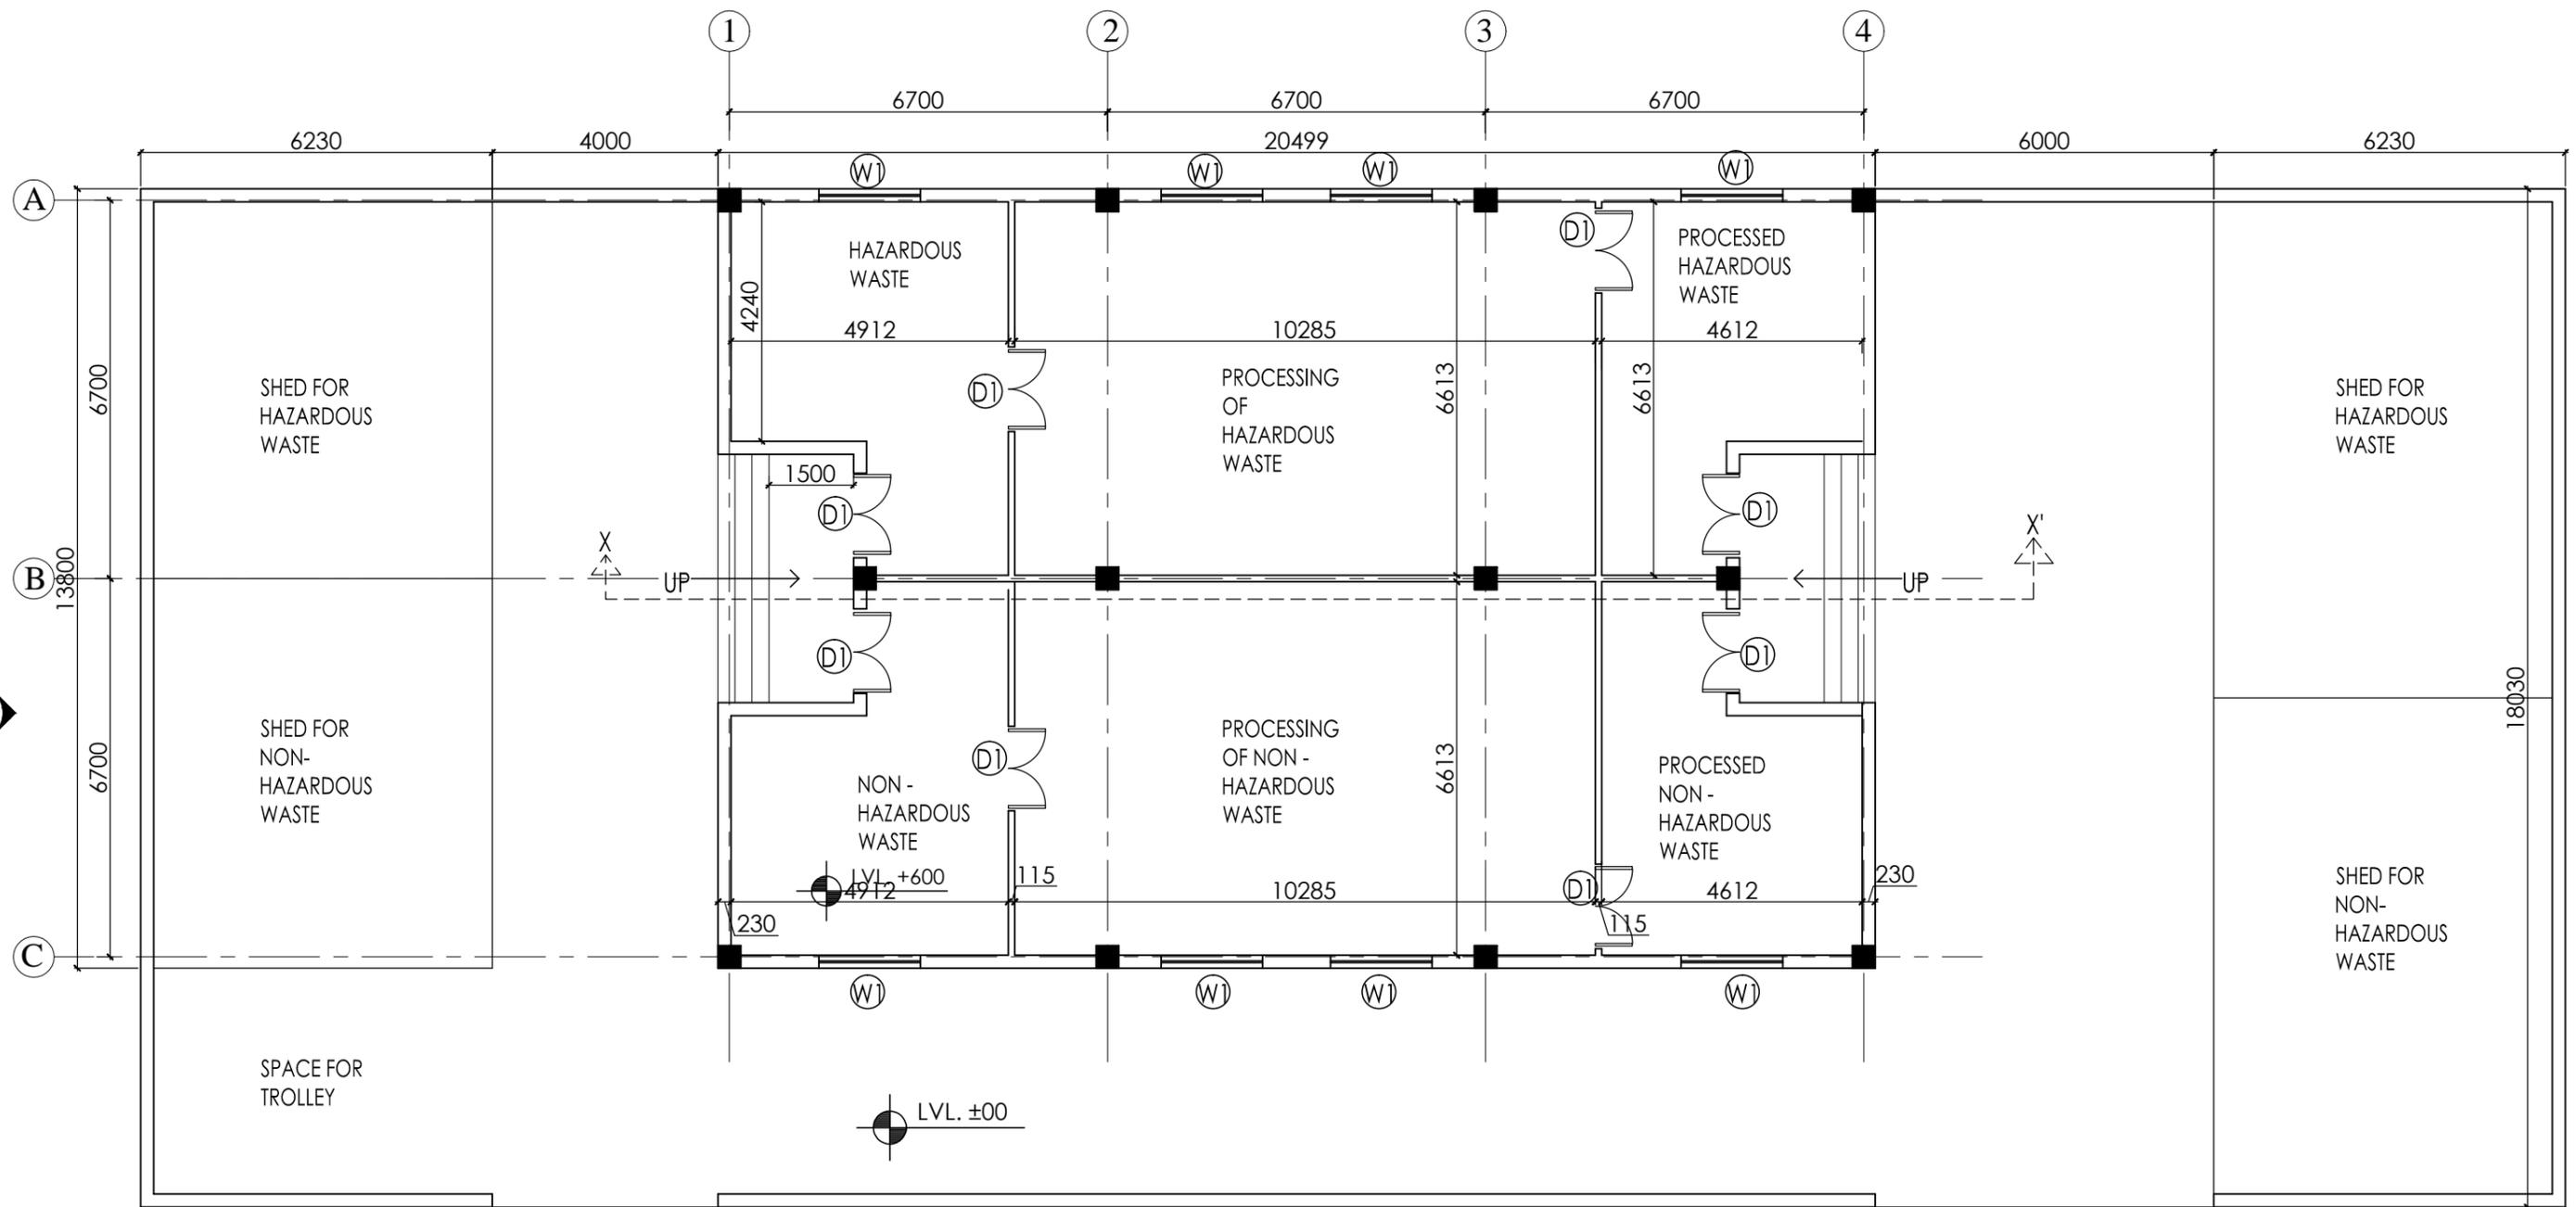

WASTE MANAGEMENT
AREA = 282.88 SQ.MT.

